


HAMILTON-C2/C3 Circuit setup, Dual Limb, Adult/Ped

Setup instructions for dual limb breathing circuit for adult and pediatric patients

Installing the expiratory valve


Refer to the figure below.

1. Holding the expiratory valve housing, seat the silicone membrane onto the housing (1). The metal plate must face up and be visible.
2. Position the housing in the expiratory port (2) and twist clockwise until it locks into place (3).

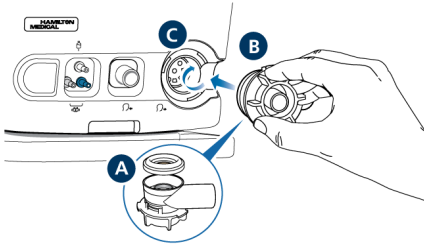

Connecting a bacteria/virus filter

- ▶ To prevent retrograde contamination of the ventilator and contamination of the environment, be sure to connect bacteria/viral filters (1) between the patient and the inspiratory and expiratory ports.




Connecting a mainstream CO2 sensor

Refer to the figure at the top of the next column.


1. Connect the sensor cable to the CO2 port (1) on the ventilator.
2. Attach the CO2 sensor (2) to the airway adapter (3), aligning the arrows on both components.

Press the components together until they click.

Connecting a mainstream CO2 sensor (cont.)

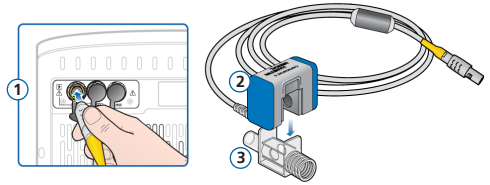

3. When connecting a CO2 sensor for the first time (or when prompted), calibrate the sensor/adapter.*
4. Connect the sensor/adapter (4) to the breathing circuit in a vertical position as follows:




5. Secure the cable safely out of the way.

Be sure to enable the CO2 sensor before use in the System > Sensors On/Off window.

Connecting the flow sensor

NOTE. To prevent inaccurate readings, ensure the flow sensor tubing is not kinked.


1. Insert a flow sensor (1) into the breathing circuit in front of the patient connection.




2. Attach the blue and clear tubes to the flow sensor connection ports on the ventilator.

The blue tube attaches to the blue connection port. The clear tube attaches to the silver connection port.

3. Calibrate the flow sensor and perform the Tightness test.*



* For details, see the HAMILTON-C2/C3 Preoperational Check Quick Reference Card (PN ELO2020-118-TW).

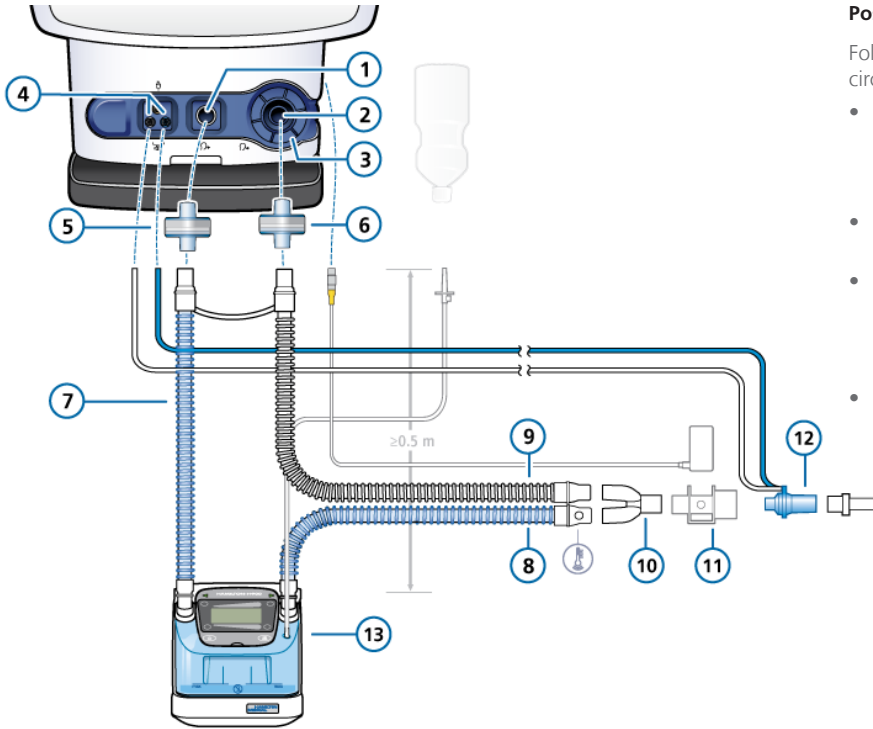


Positioning the breathing circuit

Follow these guidelines for positioning the assembled breathing circuit:

- After assembly, position the breathing circuit so that the limbs/tubing will not be pushed, pulled, or kinked as a result of a patient's movement, transport, or other activities, including scanner bed operation and nebulization.
- Position the ventilator, including the patient support arm, well back from the breathing circuit Y-piece.
- Position the flow sensor upright, with the patient end facing downward (see below).

Ideally, the flow sensor should be at a $\geq 45^\circ$ angle relative to the floor.

- Ensure there is no undue stress placed on any tubing or cables.



1	To patient inspiratory port	7	Inspiratory limb to humidifier	10	Y-piece
2	From patient expiratory port	8	Heated inspiratory limb with temperature sensor, to patient	11	CO ₂ adapter/sensor
3	Expiratory valve set	9	Heated expiratory limb	12	Flow sensor
4	Flow sensor connection ports			13	Humidifier
5, 6	Bacterial/viral filter				

